

CLOSED LOOP MODEL FOR BLOOD GLUCOSE REGULATION SYSTEM USING LABVIEW

Nalini M* Balaji V** and Gayathiri R***

Abstract: Diabetes mellitus (DM), commonly referred to as diabetes, is a group of metabolic diseases in which there are high blood sugar levels over a prolonged period. If not regulate the glucose level then it will cause the serious damage to heart, kidneys, eyes and nerves. Pancreas produces insulin to absorb the glucose. If insulin secreted is very less the excess glucose enters into the blood stream and leading to diabetes. The proposed system is, continuously monitor glucose, and insulin will be injected using insulin pump which is known as artificial pancreas. The food we take is converted into glucose. So, meal intake will greatly affect the glucose levels, in this paper a closed loop model is developed based on Bergman's minimal model and meal intake is introduced as a disturbance then the control action is performed using Fuzzy and PID controller using LABVIEW software. So, from this if the glucose concentration exceeds/decreases, above/below a certain point necessary control action will be taken.

Keywords: Fuzzy logic controller, PID controller, Lab view, Diabetes.

1. INTRODUCTION

Diabetes is a serious complex condition which can affect the entire body. Diabetes requires daily self care and if complications develop, diabetes can have a significant impact on quality of life and can reduce life expectancy. There are different types of diabetes all types are complex and serious. The three main types of diabetes are Type 1, Type 2 and Gestational diabetes. When human body consumes meal then the glucose level raises from basal value and the pancreatic β cells produce insulin to regulate the glucose level but in diabetic patients the insulin will not be produced. In open loop system the glucose level is measured and based on the value a predetermined insulin dose will be taken which is not based on the instantaneous change of glucose but in closed loop control the sensor monitors the glucose level continuously based on that the controller will suggest the amount of insulin so that the glucose level will be regulated.

The closed-loop insulin delivery system is composed of three essential components a stable glucose sensor for measuring the glucose concentration, a control system regulating external insulin infusion based on the glucose-insulin system and a safe and stable insulin pump. In this closed loop control a feedback is taken from the body by placing the sensor which senses the glucose level. The output of the sensor is given to the controller and based on the error the controller pumps the required amount of insulin to the body as shown in figure 1 The closed loop method of insulin delivery system is called as artificial pancreas.

* Research Scholar/SCSVMV University, India.

Faculty, Department of Electronics and Instrumentation Engineering/ Sri Sairam Engineering College, Email: naalsnalini@gmail.com

** Faculty of Electrical Engineering/Bahir Dar University, Email: balajiee79@gmail.com,

*** Faculty, Department of Electronics and Instrumentation Engineering/Sri Sairam Engineering College, Email: gayathiri.ei@sairam.edu.in

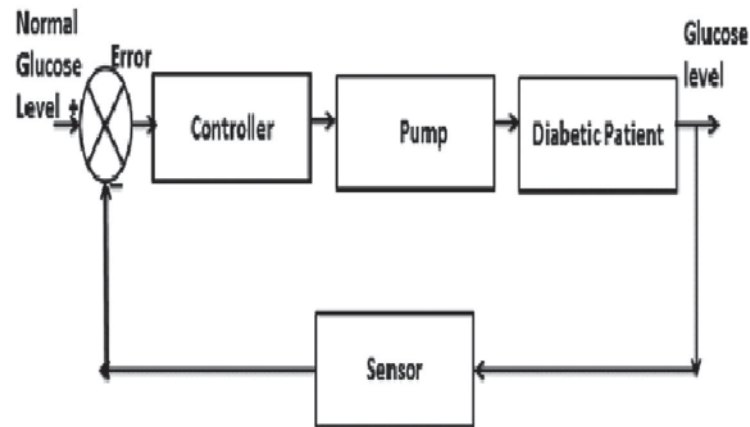


Figure 1. Closed loop control of blood glucose

From 1961 many mathematical models were derived [6, 7, 8, 9, 10, 11] which describes the relation of glucose insulin dynamics. In [12] the model developed was based on the patient's data. Based on these mathematical models many control algorithms were developed to control blood glucose [13, 14, 15, 16]. This paper takes Bergman's minimal model and includes meal as disturbance then the controller will be simulated using PID and Fuzzy Logic Controller. The paper is organized as follows section II describes the mathematical modeling. Section III describes simulation using LABVIEW. Section IV includes results and discussion finally conclusion and future scope.

2. MATHEMATICAL MODELING FOR GLUCOSE INSULIN REGULATION SYSTEM

The input is the measured plasma insulin concentration $y(t)$ following the intravenous glucose injection, while the output is corresponding measured glucose concentration $x(t)$. The insulin concentration $y(t)$ acts through a remote compartment so that effective Insulin concentration $y_{eff}^{(t)}$ is given by,

$$\frac{dy_{eff}}{dt} = k_2 y^{(t)} - k_3 y_{eff}^{(t)} \quad (1)$$

Where k_2 and k_3 represents the fractional rate parameter for insulin transport into and elimination in the remote compartment. This compartment is not directly measurable. The rate of change of glucose in blood plasma is given by

$$\frac{dx}{dt} = (\text{Net rate of glucose production by liver} \\ - \text{Rate of glucose utilization by other tissues})$$

Net rate of glucose production by the liver

$$= B_0 - k_5 x(t) - k_6 y_{eff}(t)x(t)$$

Rate of glucose utilization by other tissues

$$= R_{d0} + k_3 x(t) + k_4 y_{eff}(t)x(t)$$

In the equation B_0 represents the rate of glucose production by the liver. It is assumed to be proportional to an insulin independent component (through rate constant k_5) and an insulin dependent component k_6 . Similarly the rate of glucose utilization by non-hepatic tissues is assumed to have a constant component which is proportional to glucose concentration and sensitive to both glucose and effective insulin concentration. Then

$$\frac{dx}{dt} = [B_0 - R_{d0}] - [k_5 + k_3]x(t) - [k_6 + k_4]y_{eff}(t)x(t) \quad (2)$$

$y_{eff}^{(0)}$ is not measurable a further reduction in parameterization can be achieved by considering new variable $z(t)$ which is proportional to $y_{eff}^{(0)}$:

$$z(t) = [k_6 + k_4]y_{eff}(t) \quad (3)$$

$$\frac{dz}{dt} = -p_2z(t) + p_3y(t) \quad (4)$$

$$\frac{dx}{dt} = p_4 - p_1x(t) - z(t)x(t) \quad (5)$$

Where

$$p_1 = (k_1 + k_5), p_2 = k_3, p_3 = k_2(k_4 - k_6), p_4 = B_0 - R_{d0}$$

the unknown parameter values are taken from [17]. An optimization algorithm is used for calculating other four unknown parameters. The estimated values of unknown parameters using m-file are $P_1 = 0.049$, $P_2 = 0.091$, $P_3 = 8.96 \times 10^{-5}$ and $P_4 = 4.42$.

2.1 Software Realization Using Labview

In LabVIEW software simulation loop, integrator block, signal generator block, PID block and Fuzzy blocks are available in control design and simulation tool kit. In the front panel of LABVIEW, the meal disturbance, glucose concentration, insulin concentration and regulated insulin graphs are visualized using graphs and in the block diagram the modeling equations developed for diabetic persons are implemented. Here the simulation using two logics are performed and they are **PID** and **Fuzzy logic**.

2.2 PID logic implementation

The glucose value changes every time according to the consumption of food this disturbance was added to the process as a random signal. Every time the glucose value is measured and corrective insulin was injected to the body and this insulin was controlled by PID controller. The figure 2 shows the PID implementation.

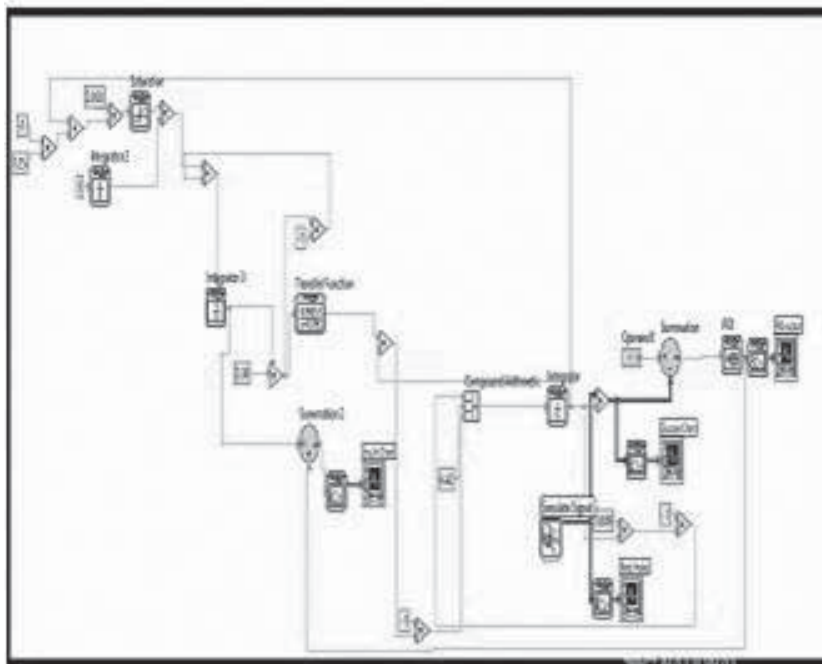


Figure 2. PID Implementation

After simulation the outputs were shown in graphs as PID output which gives the insulin rate but the response has some delay which is because of controller action and sensor delay.

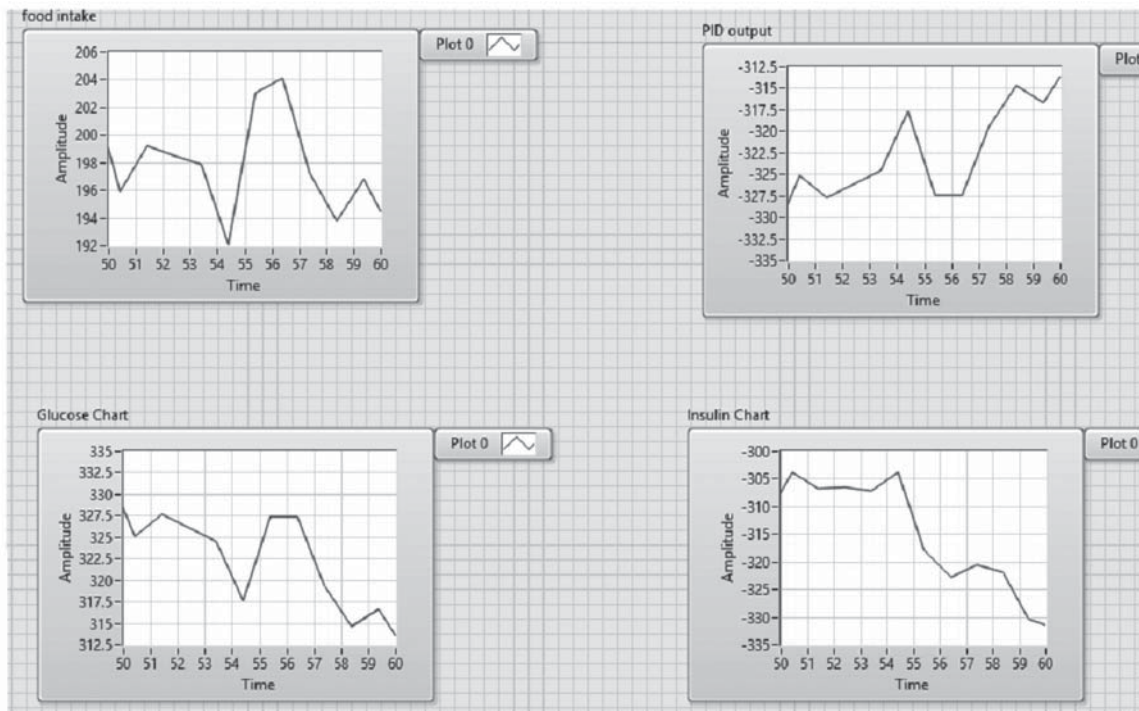


Figure 3. PID output

Thus whenever the glucose changes the insulin will also changes accordingly. Figure 3 shows the output graphs consists of meal disturbance, measure glucose, insulin chart before without PID controller, insulin chart with PID controller.

2.3 Fuzzy Implementation

The controller used here is FUZZY controller (Mamdhani type). The Linguistic variables are measured glucose and insulin. The membership functions were defined for the linguistic variables then the rules formed. The figure 4 shows the simulation using FUZZY controller.

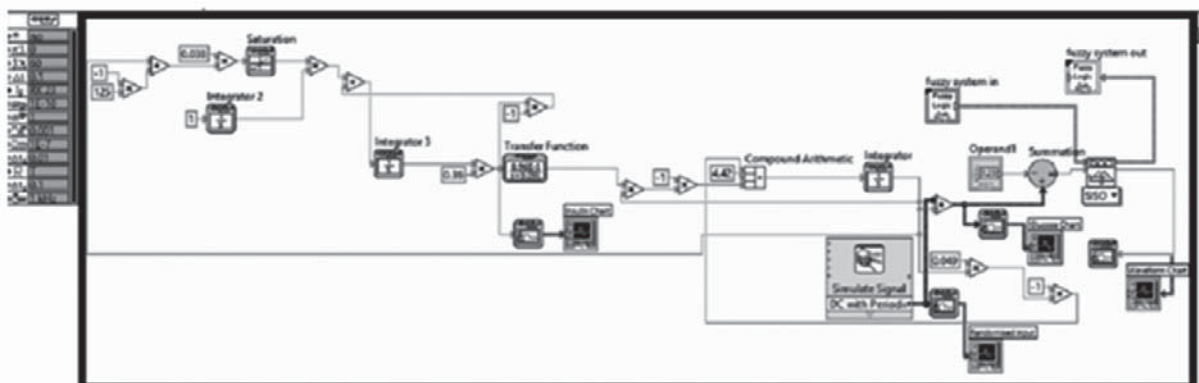


Figure 4. FUZZY implementation

Then the results were shown in figure 5 which has the graph for fuzzy controlled insulin output.

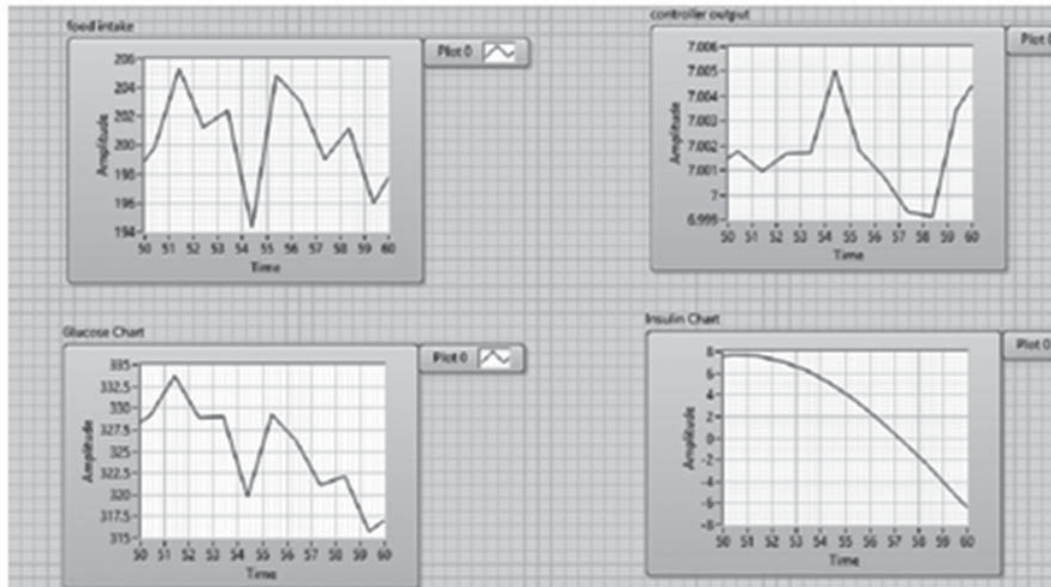


Figure 5. Fuzzy output

3. RESULTS AND DISCUSSIONS

When glucose falls below a certain level i.e 70 mg/dl then it is called hypoglycemia and when it exceeds 130 mg/dl then it is called hyperglycemia. In this simulation both the extremes are not occurred. Table 1 will give the comparison between PID and Fuzzy output.

Table 1.
Validation of results

Controllers Used	Delay Time (Td) sec	Rise Time (Tr) sec	Peak Overshoot(Mp) %	% Steady State Error (Ess)
PID Controller	0.0242	0.04	15.9	1.6
FUZZY logic controller	0.024	0.04	8.1	0

4. CONCLUSION AND FUTURE WORK

This paper developed the PID and Fuzzy controller for artificial pancreas. It is inferred from the results that the fuzzy controller has better performance than PID controller. Another advantage of fuzzy controller is by increasing the membership functions and rules the performance can be improved. The future work includes addition of other dynamics in glucose insulin models can improve the performance and other controllers also can be included. This is an offline analysis and the online analysis can also be tried.

References

1. Srinivas, P., and P. DurgaPrasada Rao. "closed loop model for glucose insulin regulation system using labview." *International Journal of Instrumentation and Control Systems* Vol.2, No.4, October 2012
2. Kanderian, Sami S., et al. "Identification of intraday metabolic profiles during closed-loop glucose control in individuals with type 1 diabetes." *Journal of diabetes science and technology* 3.5 (2009): 1047-1057.
3. Pinky Dua, Francis J. Doyle, and Pistikopoulos, "Model-Based Blood Glucose Control for Type 1 Diabetes via Parametric Programming", *IEEE Transactions on Biomedical Engineering*, vol.53, pp.1478-1491, August 2006.
4. Fernandez, M. Acosta, D. Villasana, M. Streja, D., "Enhancing Parameter Precision and the Minimal Modeling Approach in Type I Diabetes", *Proc. of 26th Annual Int. Conf. of IEEE Eng. in Biomedicine Soc.*, San Francisco, CA, USA, pp. 797-800, September 2004.

5. L. Eiselein , H. J. Schewartz and J. C. Rutledge, “The challenge of type 1diabetes mellitus”, *ILAR J.*, vol. 45, no. 3, pp. 231-236, 2004
6. C. Cobelli , G. Federspil , G. Pacini , A. Salvan and C. Scandellari, “An integrated model of blood glucose dynamics control”, *Math. Biosci.*, vol. 58, pp.27-60, 1982.
7. J. V. Santiago , A. H. Clemens , W. C. Clarke and D. M. Kipnis, “Closed- loop devices for blood glucose control in normal and diabetic subjects”, *Diabetes*, vol. 28, pp. 71-84, 1979.
8. Ackerman, E., Gate wood, L.C., Rosevear, J. W. and Molnar, G.D., “Model studies of blood glucose regulation”, *The Bulletin of Mathematical Bio Physics*, 27(suttl.), 21,1965.
9. Bergman, R.N., Philips, L.S and Cobelli, C., “Physiologic evaluation of factors controlling glucose tolerance in man”, *A Journal of clinical investigation*, 68, 1456, 1981.
10. Cobelli, C. and Ruggeri, A., “Evaluation of portal/peripheral route end of algorithms for insulin delivery in closed loop control of glucose in diabetes- A modelling study ” *IEEE transactions on Biomedical Engineering*, BME-30: 90-103,1983.
11. Puckett, W.R, “Dynamic Modeling of Diabetes Mellitus” PhD. Dissertation, Department of Chemical Engineering, University of Wisconsin-Madison, 1992.
12. Puckett, W.R and Lightfoot, E.N., “A Model for Multiple Subcutaneous Insulin Injections Developed from Individual Diabetic Patient data” *American journal of Physiology*,269(Endocrinology metabolism 32), E115,1995.
13. Ch. Li and R. Hu, “Simulation study on blood glucose control in diabetics”, *Proc. IEEE Int. Conf. on Biomed. and Bioinf. Eng.*, 2007, pp. 1103-1106.
14. F. Chee, T. L. Fernando, A. V. Savkin, and V. Heeden, “Expert PID control system for blood glucose control on critically ill patients”, *IEEE Trans. Boimed. Tech.* Vol. 7, No. 4, 2003.
15. Z. H. Lam, J. Y. Hwang, J. G. Lee, J. G. Chase, and G. C. Wake, “Active insulin infusion using optimal and derivative-weighted control”, *Medical Engineering & Physics.* Vol. 24, 2002, pp. 663-672.
16. K. H. Kientiz and T. Yoneyame, “A robust controller for insulin pupms based on H-infinity theory” *IEEE Transaction on Boimedical Engineering*, Vol. 40, 1993, pp. 1133-1137.
17. Michael C. K. Khoo, “Physiological control systems:Analysis,simulation and estimation”, *The Institute of Electrical and Electronics Engineers, Inc.* 3 Park Avenue, 17th Floor, New York, NY 10016-5997.